

UTI-6 for imc ARGUSfit

6-channel measurement module for
voltage, current, temperature (RTD) and resistance (NTC)



The UTI-6 module belonging to the imc ARGUSfit series is a 6-channel measurement amplifier that can be used in conjunction with an imc ARGUS system (or base unit) to which it is directly docked with its housing.

Individually isolated, configurable differential channels capturing:

- Voltage (25 mV to 60 V)
- Current (20 mA sensors)
- Temperature (PT100, PT1000)
- Resistance (e.g. NTC)


Highlights

- Per-channel isolated measurement inputs, individual filtering and ADCs
- Sensor supply (for active voltage-fed sensors), individually isolated and adjustable
- 40 kHz bandwidth at max. 100 kSps/channel sampling rate
- Measurement ranges and sampling rates individually selectable (in steps of 1, 2, 5)
- 24-bit digitization, internal processing and data resolution
- Robust, compact and miniaturized: click mechanism for imc ARGUSfit systems

Typical applications

- Robust data acquisition for mobile or stationary applications and for test benches
- General voltage signals, including vehicle battery voltage (up to 60 V) and current measurements with external shunts (down to 25 mV)
- Active voltage-fed sensors
- Industrial sensors (20 mA) for arbitrary physical variables
- Temperature measurement with resistance-based sensors (PT100, PT1000, NTC)

imc ARGUSfit: Flexible modular platform for fast measurement systems

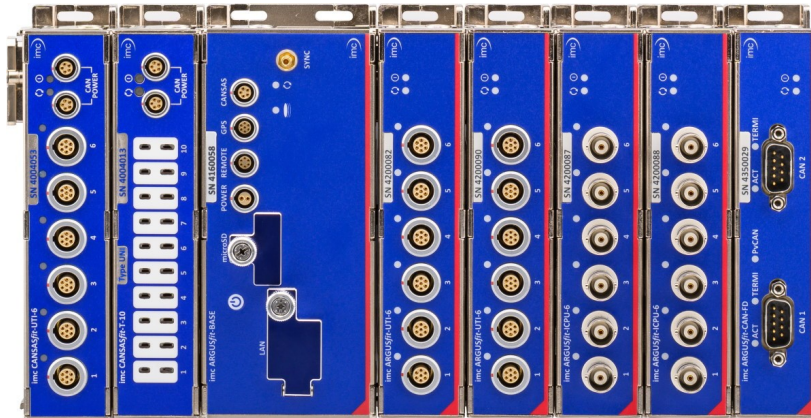


Based on an imc ARGUSfit base unit, imc ARGUSfit measurement amplifier and interface modules can be combined to form complete systems by means of a robust click mechanism, which can even integrate imc CANSASfit modules. The click connectors provide the electrical connection to the power supply and system bus.

For expansion to decentralized distributed topologies, the fast internal ARGFT system bus can be converted to fiber optic cables by means of a clickable fiber converter module.



The entire system can be controlled via a common Ethernet connection (LAN/WLAN) with a PC (imc STUDIO software) and can be networked and operated synchronously and uniformly with all other imc data acquisition instrument series. Furthermore, it can also be operated autonomously and stand-alone without PC with data storage on microSD.

Dimensions

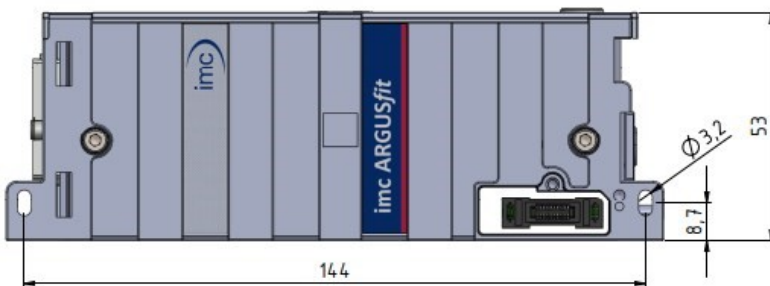

imc ARGUSfit UTI-6

Module shown in standard operating position (terminal connections upwards)

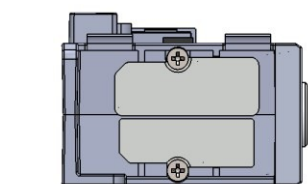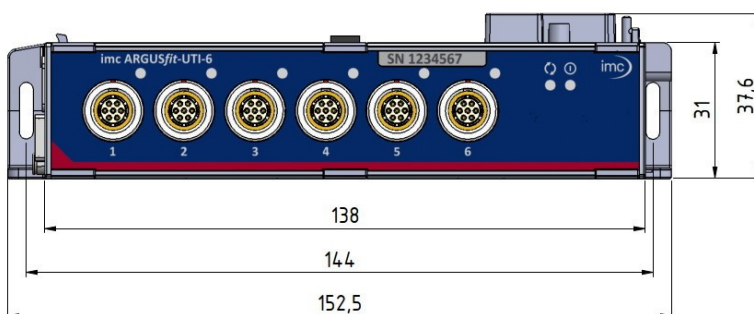

left module panel with parking position for the covers of the module connectors

Overview of the available variants

Order Code	Properties	article no.
ARGFT/UTI-6-SUP	voltage amplifier with sensor supply (-40°C... +85°C)	11400206
ARGFT/UTI-6-SUP-EC	variant for extended condensation	11410202

Included accessories

Documents
Getting started with imc ARGUSfit (one copy per delivery)
Device certificate
Miscellaneous
6x ACC/CAP-LEMO.1B, 13500233 (protective cover for LEMO.1B sockets)

Optional accessories

Connector: signals		
ACC/FGG.1B.307-5.3-6.2	plug for the signal connection (FGG series, IP50)	13500096
ACC/FEG.1B.307-3.1-4.2	plug for the signal connection (FEG series, IP54)	13500262
ACC/FGG.1B.307-TERMINAL	screw terminal plug LEMO.1B, 7 pin (FGG series) LEMO plug with integrated screw terminal adaptor (7 pin + shield)	13500418

Fiber-Converter Set		
ARGFT/FIBER-CONVERTER-SET	Media converter for the ARGUS system bus Includes: 2 converter modules, 2x SFP+ transceiver, 5 m fiber optic cable, AC/DC power adaptor and a power plug	11400225


Mounting accessories		
CANFT/BRACKET-DIN	Mounting on DIN-Rail (top hat rail) for imc ARGUSfit and imc CANSASfit	12100029
CANFT/BRACKET-MAG	Mounting with magnet system for imc ARGUSfit and imc CANSASfit	12100030

Documents		
SERV/CAL-PROT	Calibration protocol per amplifier imc manufacturer calibration certificate with measurement values and list of calibration equipment used (pdf).	150000566
SERV/CAL-PROT-PAPER	Calibration protocol per amplifier (paper print) imc manufacturer calibration certificate with measurement values and list of calibration equipment used with signature and seal.	150000578

Device certificates and calibration protocols: Detailed information on certificates supplied, the specific contents, underlying standards (e.g. ISO 9001 / ISO 17025) and available media (pdf etc.) can be found on our website, or you can contact us directly.

Technical Specs - ARGFT/UTI-6

General

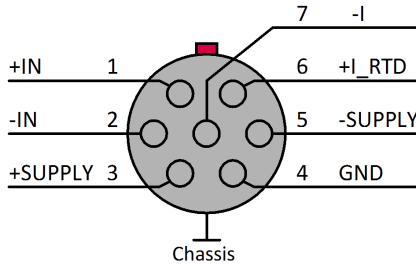

Inputs, measurement mode			
Parameter	Value typ.	min. / max.	Remarks
Inputs	6		
Measurement mode	voltage current resistance temperature PT100/PT1000		4-wire
Connector / socket Measuring input LEMO pin configuration	compatible socket type LEMO.1B 7-pin measuring input		recommended plug FEG.1B.307
Module connector			for the supply and system bus of directly connected modules without further cables, see data sheet of ARGFT base unit
	Click-connection (covering caps)		

Sampling rate, Bandwidth, Filter			
Parameter	Value typ.	min. / max.	Remarks
Sampling rate		≤100 kHz	configurable, individually per channel
Bandwidth	0 Hz to 40 kHz 0 Hz to 30 kHz		sampling rate 100 kHz, AAF filter -3 dB 0.1 dB
Filter Type Characteristic Cut-off frequency Order Anti-aliasing filter	low pass Mean, Butterworth, Bessel, AAF 1 Hz to 20 kHz 8 th Cauer 8 th order		individual selectable; mean and AAF: adapted automatically, according to selected output rate -3 dB, 1 - 2 - 5 steps digital filter in addition to hardware filter with $f_{\text{cut-off}} = 0.4 \cdot f_s$; f_s : output rate
Resolution	24 Bit		output: 32 Bit Float (24 Bit mantissa)

Isolation		
Parameter	Value	Remarks
Isolation	galvanically isolated	
channel-to-case (CHASSIS)	±60 V	test voltage: ±300 V (10 s)
channel to power supply	±60 V	test voltage: ±300 V (10 s)
channel-to-channel	±60 V	test voltage: ±300 V (10 s)

Power supply of the module			
Parameter	Value typ.	min. / max.	Remarks
Input supply voltage		7 V to 50 V DC 9.5 V to 50 V DC	operating upon power up power supply via base unit, fiber converter or UPS module
Power consumption	3 W	3 W	sensor supply not loaded
	1.5 @ 12 V 5.7 @ 12 V	7 W	sensor supply loaded
Isolation		±60 V	to case (CHASSIS), isolation impedance ≥1 MΩ

Pass through power limits for directly connected modules (click-mechanism)		
Parameter	Value	Remarks
Max. current	5 A	at 85 °C current rating of click connector to ARGFT modules
	60 W at 12 V DC 120 W at 24 V DC	typ. DC vehicle voltage AC/DC power adaptor and installations

LED		
Parameter	Value	Remarks
Power-LED green	 power active	
Status-LED green blue magenta yellow red	 multicolor operating, run init, etc. firmware update prepare configuration error	global status of module
Channel-Status-LED off green red red	bicolor channel passive channel active over-range error error	status for each channel >5 % over nominal range see manual for detailed information

Sensor supply			
Parameter	Value typ.	min. / max.	Remarks
Output voltage	$\pm 15\text{ V}, \pm 12\text{ V}, \pm 10\text{ V}, \pm 7.5\text{ V},$ $\pm 5\text{ V}, \pm 4\text{ V}, \pm 3.5\text{ V}, \pm 3.3\text{ V}, \pm 3\text{ V}, \pm 2.5\text{ V}$		referenced to GND; arbitrary for each channel
Short-Circuit-Proof	unlimited duration		protection for module and each channel
Error of output voltage		$\pm 2\%$ $0.01\%/K \cdot \Delta T_a$	$\Delta T_a = T_a - 25^\circ\text{C} $; with T_a = ambient temperature
Max. Output current	150 mA		
Output power per channel		0.5 W 0.4 W	bipolar supply with symmetric load unipolar supply or asymmetric load
per module		2 W	
Output impedance	0.6 Ω		

Measurement modes


Voltage measurement			
Parameter	Value typ.	min. / max.	Remarks
Input range	$\pm 60\text{ V}, \pm 50\text{ V}, \pm 25\text{ V}, \pm 10\text{ V}, \pm 5\text{ V},$ $\pm 2.5\text{ V}, \pm 1\text{ V}$ to $\pm 25\text{ mV}$		input range $\pm 60\text{ V}$ (nominal working voltage according to low voltage directive SELV) is valid up to 100 V without limitation
Max. Over Voltage	$\pm 200\text{ V}$		differential input voltage
Input coupling	DC		
Input impedance	1 M Ω 20 M Ω	$\pm 1\%$ $\pm 1\%$	measurement ranges $\geq \pm 5\text{ V}$ or device off measurement ranges $\leq \pm 2.5\text{ V}$
Gain error	0.008% $+ 0.0004\%/K \cdot \Delta T_a$	0.02% $+ 0.001\%/K \cdot \Delta T_a$	of reading $\Delta T_a = T_a - 25^\circ\text{C} $; with T_a = ambient temperature
Offset error	0.003% $+ 0.00006\%/K \cdot \Delta T_a$	0.02% or 10 μV $+ 0.001\%/K \cdot \Delta T_a$	of range whichever is greater $\Delta T_a = T_a - 25^\circ\text{C} $; with T_a = ambient temperature
Bandwidth ranges $\pm 60\text{ V}$ to $\pm 100\text{ mV}$ ranges $\pm 50\text{ mV}$ to $\pm 25\text{ mV}$	0 Hz to 40 kHz 0 Hz to 30 kHz 0 Hz to 30 kHz 0 Hz to 8 kHz		-3 dB 0.1 dB -3 dB 0.1 dB
IMRR (Isolation mode rejection ratio)	90 dB 130 dB		50 Hz measurement ranges $\geq \pm 5\text{ V}$ measurement ranges $\leq \pm 2.5\text{ V}$
Noise	1 mV _{rms} 16 μV _{rms} 14 μV _{rms}		sampling rate = 100 kHz; filter = AAF; resolution = 32 bit float; ranges: 60 V, ..., 5 V 2.5 V 1 V, ..., 25 mV

Current measurement			
Parameter	Value typ.	min. / max.	Remarks
Input range	±20 mA		
Overload	±100 mA		
Input coupling	DC		
Input impedance	25 Ω	±1%	
Gain error		0.02% + 0.002%/K·ΔT _a	of the measured value ΔT _a = T _a - 25°C ; with T _a = ambient temperature
Offset error		0.01% + 4 nA/K·ΔT _a	of range ΔT _a = T _a - 25°C ; with T _a = ambient temperature
Bandwidth	0 Hz to 48 kHz 0 Hz to 30 kHz		-3 dB 0.1 dB

Resistance measurement			
Parameter	Value typ.	min. / max.	Remarks
Input range	100 kΩ, 50 kΩ, 25 kΩ, 10 kΩ, ..., 100 Ω		
Overvoltage protection	±30 V		
Input coupling	DC		
Gain error		0.02% + 0.002%/K·ΔT _a	of the measured value ΔT _a = T _a - 25°C ; with T _a = ambient temperature
Offset error		0.01% + 0.003%/K·ΔT _a	of range ΔT _a = T _a - 25°C ; with T _a = ambient temperature
Bandwidth	0 Hz to 28 kHz 0 Hz to 10 kHz		-3 dB 0.1 dB

RTD measurement			
Parameter	Value typ.	min. / max.	Remarks
Temperature Sensors	Resistance Temperature Detectors (RTDs) PT100, PT1000		4-wire configuration
Input range	-200°C to 850°C -200°C to 250°C		
Overvoltage protection	±60 V		
Input coupling	DC		
Supply Current	0.88 mA 0.7 mA		PT100; P _{dis} < 0.3 mW PT1000; P _{dis} < 1.9 mW
Measurement error PT100, PT1000			
-200°C to 0°C	0.001 K	0.05 K	
0°C to 100°C	0.001 K	0.1 K	
100°C to 300°C	0.002 K	0.18 K	
300°C to 500°C	0.003 K	0.25 K	
500°C to 850°C	0.006 K	0.4 K	

Operating conditions

Operating conditions		
Parameter	Value	Remarks
Operating environment	dry, non corrosive environment within specified operating temperature range	
Ingress protection class	IP50	with correctly mounted covers over both module connectors
Pollution degree	2	
Operating temperature range	-40 °C to +85 °C	standard version: without condensation "-EC" version: temporary condensation allowed
Shock- and vibration resistance	IEC 60068-2, IEC 61373 IEC 60062-2-64 category 1, class A and B MIL-STD-810 Rail Cargo Vibration Exposure U.S. Highway Truck Vibration Exposure	
Extended shock- and vibration resistance	upon request	specific tests or certification upon request
Dimensions (L x W x H)	approx. 153 x 40 x 54 mm	including mounting flanges and click mechanism, see mechanical drawings 
Weight	0.33 kg	



An Axiometrix Solutions Brand

Contact imc

Address

imc Test & Measurement GmbH

Voltastr. 5

13355 Berlin

Phone: (Germany): +49 30 467090-0

E-Mail: info@imc-tm.de

Internet: <https://www.imc-tm.com>

Tech support

If you have problems or questions, please contact our tech support:

Phone: (Germany): +49 30 467090-26

E-Mail: hotline@imc-tm.de

Internet: <https://www.imc-tm.com/service-training/>

imc ACADEMY - Training center

The safe handling of measurement devices requires a good knowledge of the system. At our training center, experienced specialists are here to share their knowledge.

E-Mail: schulung@imc-tm.de

Internet: <https://www.imc-tm.com/service-training/imc-academy>

International partners

You will find the contact person responsible for you in our overview list of imc partners:

Internet: <https://www.imc-tm.com/imc-worldwide/>

imc @ Social Media

<https://www.facebook.com/imcTestMeasurement>

<https://www.youtube.com/c/imcTestMeasurementGmbH>

https://twitter.com/imc_de

<https://www.linkedin.com/company/imc-test-&-measurement-gmbh>